## This Page Is Inserted by IFW Operations and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**


Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):


- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


## IMAGES ARE BEST AVAILABLE COPY.


As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.

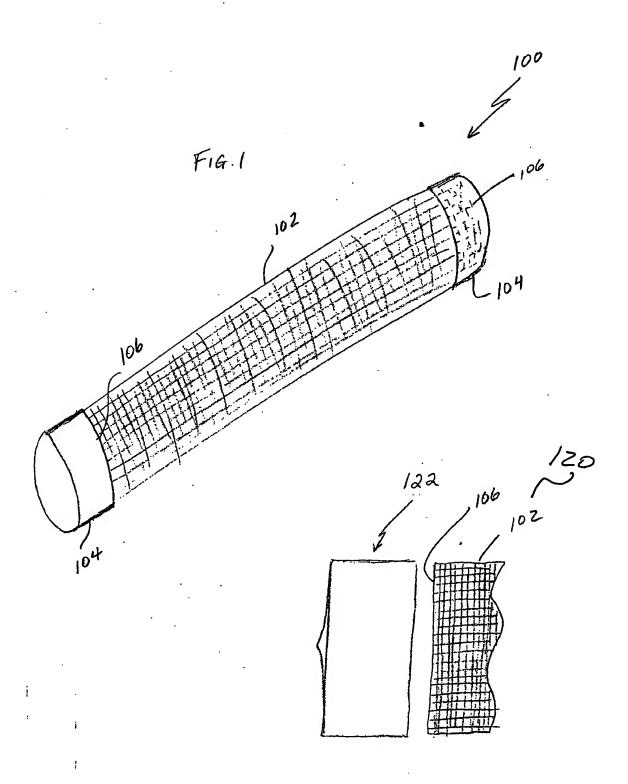


F16.2

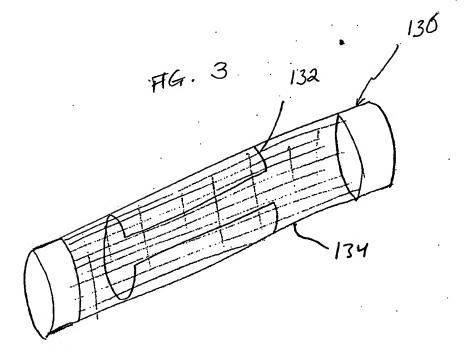


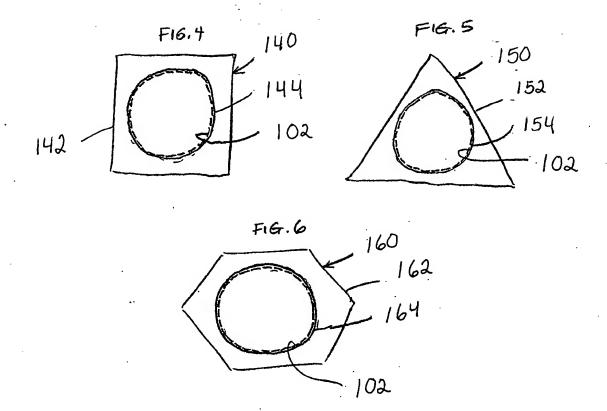


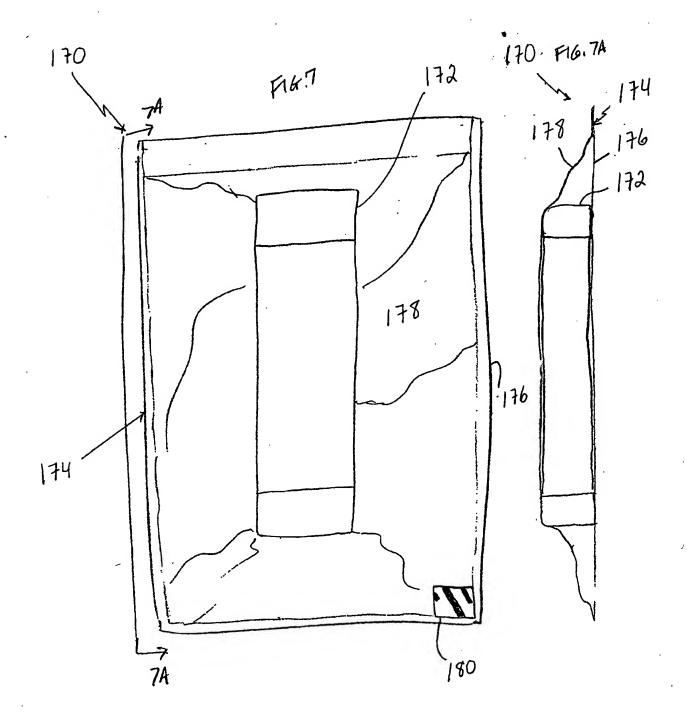


Provide a tube in a sterilized package at a point of use Open the pockage Remove the tube from the package Remove the end cap from one end of tube Place the used device in the tube Replace the end cap on the tube 214. - Remove the used devices in the take from the 276 - Place the tube containing the dovices in a both FIG. 84

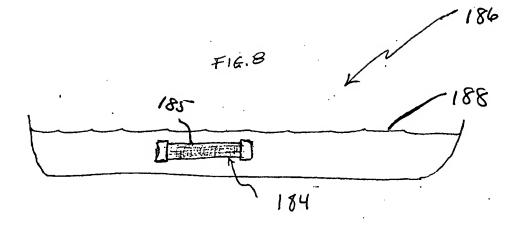

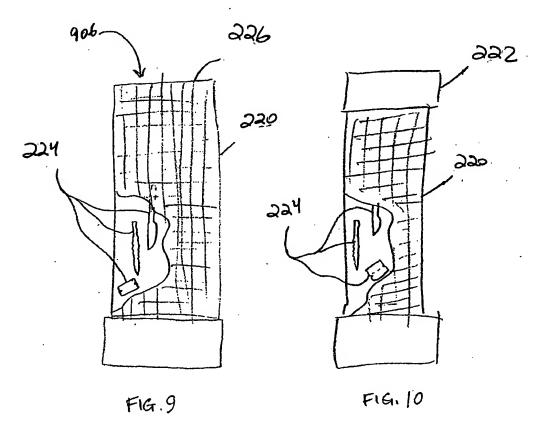

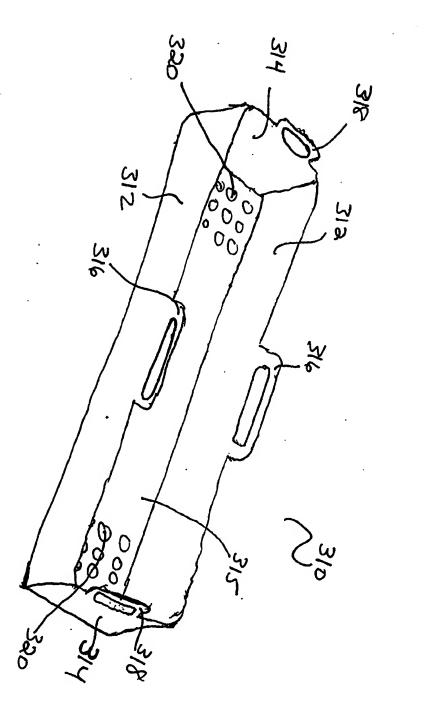



76. 1

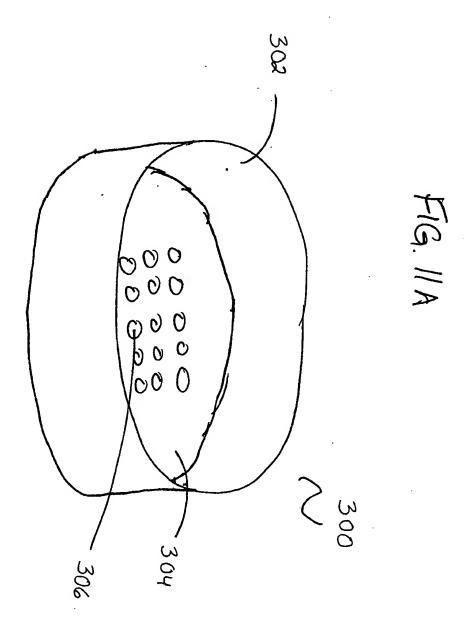

4-

\_\_\_

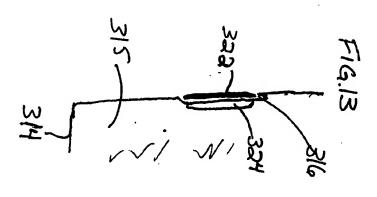

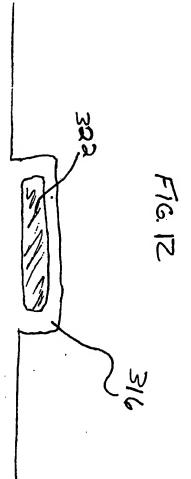




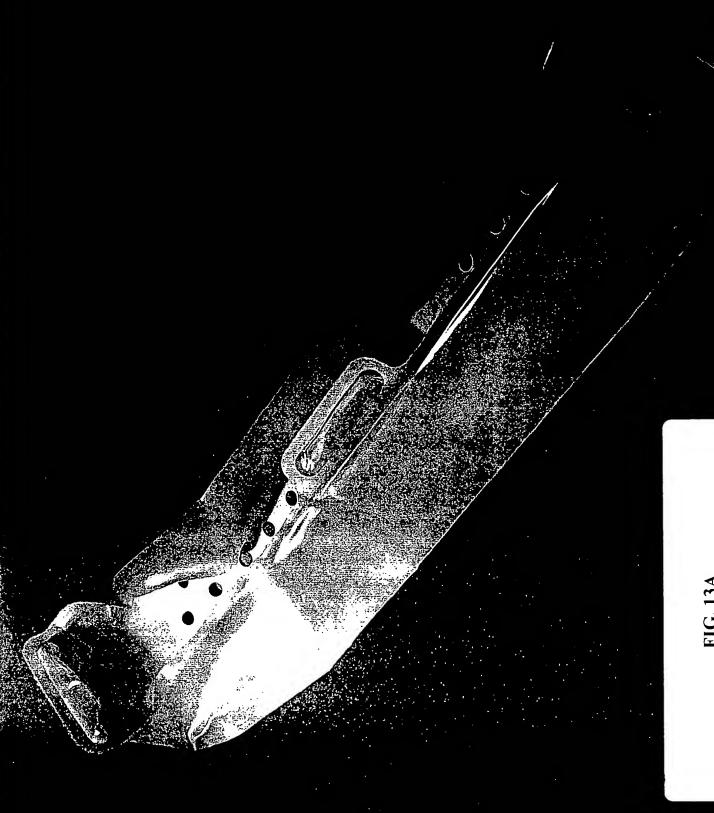



FIG. 13A

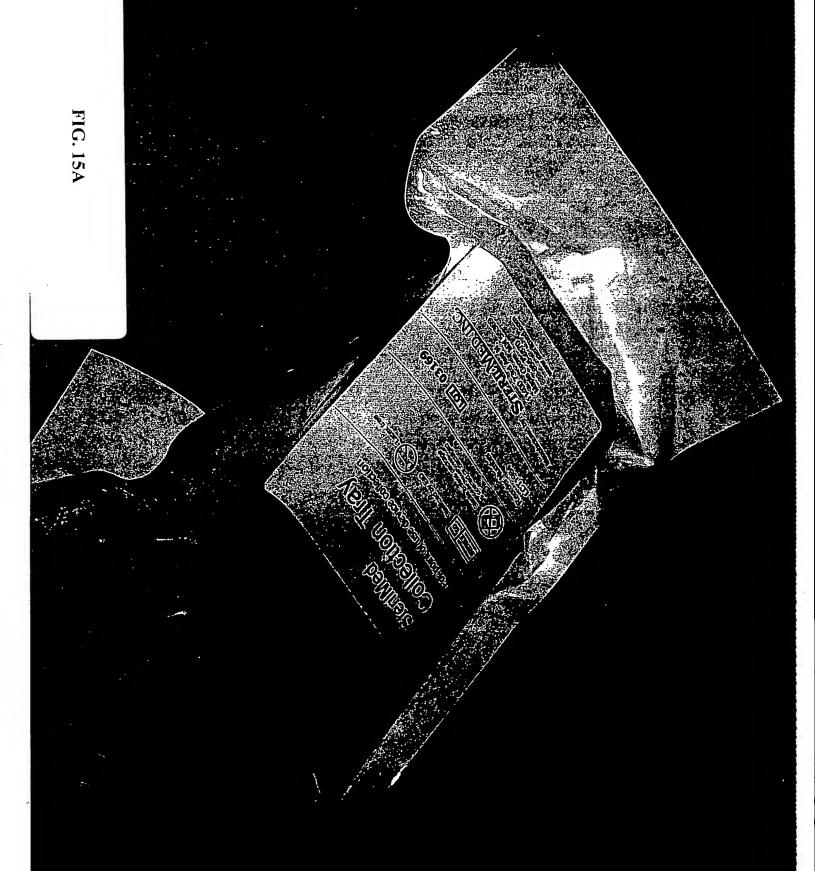


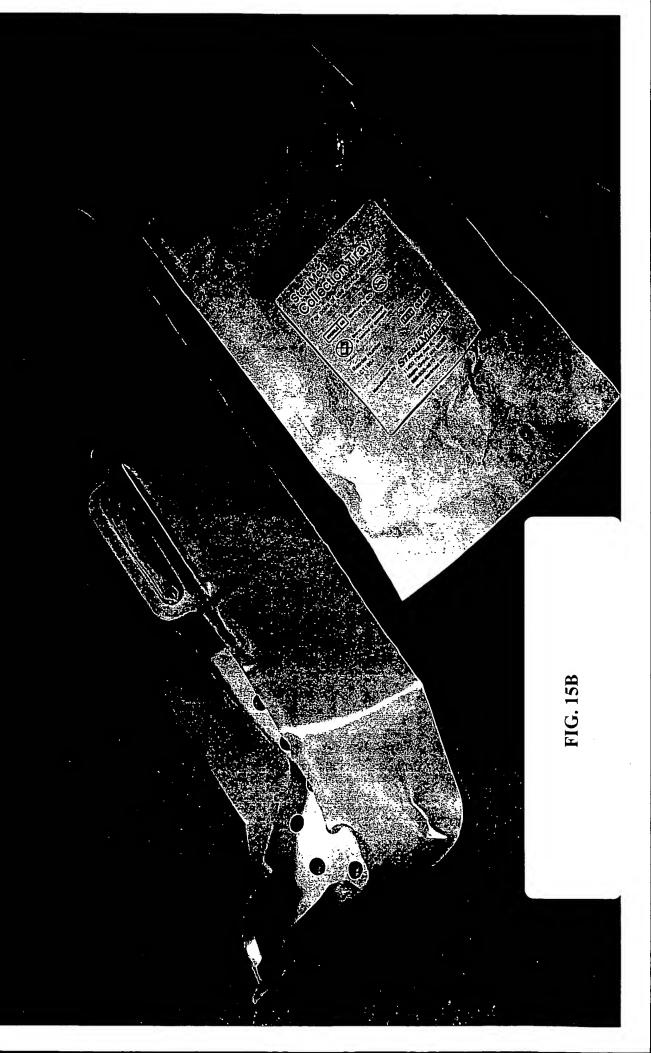

## Collection Tray

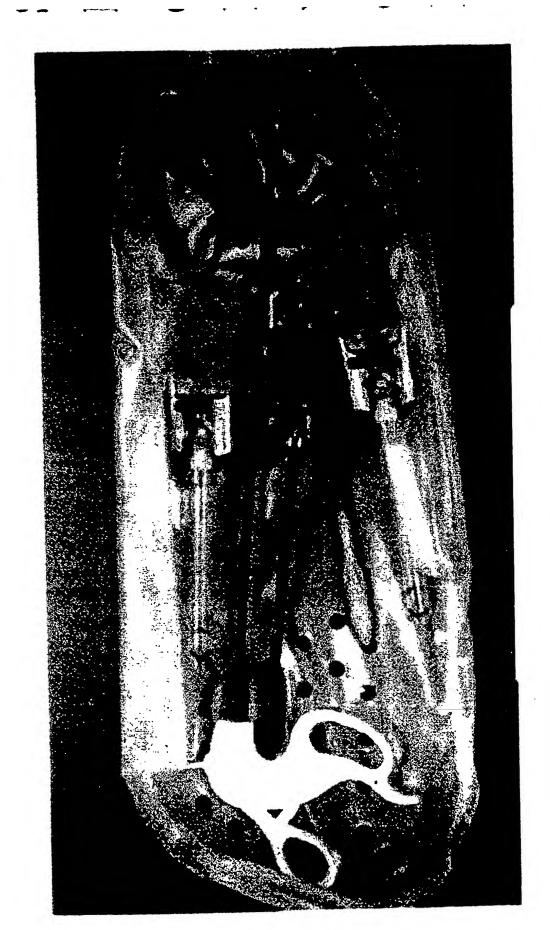

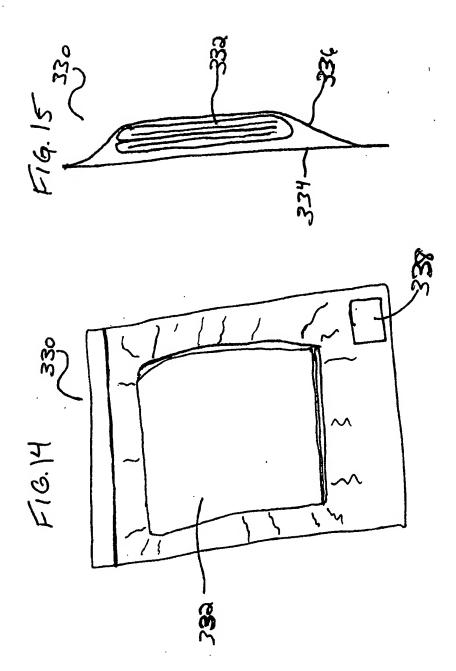

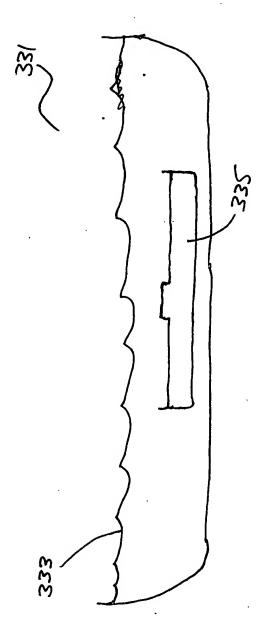

F19. 16A

